



(11) **EP 2 138 867 A1**

(12) **EUROPEAN PATENT APPLICATION**  
published in accordance with Art. 153(4) EPC

(43) Date of publication:  
**30.12.2009 Bulletin 2009/53**

(51) Int Cl.:  
**G01T 1/20 (2006.01) G01T 1/161 (2006.01)**

(21) Application number: **07806417.7**

(86) International application number:  
**PCT/JP2007/066940**

(22) Date of filing: **30.08.2007**

(87) International publication number:  
**WO 2008/136141 (13.11.2008 Gazette 2008/46)**

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC MT NL PL PT RO SE SI SK TR**

(30) Priority: **23.04.2007 JP 2007112925**

(71) Applicants:  

- **National Institute of Radiological Sciences**  
Chiba-shi, Chiba 263-8555 (JP)
- **Shimadzu Corporation**  
Kyoto-shi  
Kyoto 604-8511 (JP)

(72) Inventors:  

- **YOSHIDA, Eiji**  
Chiba-shi  
Chiba 263-8555 (JP)


- **SHIBUYA, Kengo**  
Chiba-shi  
Chiba 263-8555 (JP)
- **YAMAYA, Taiga**  
Chiba-shi  
Chiba 263-8555 (JP)
- **MURAYAMA, Hideo**  
Chiba-shi  
Chiba 263-8555 (JP)
- **KITAMURA, Keishi**  
Kyoto-shi  
Kyoto 604-8511 (JP)

(74) Representative: **Grünecker, Kinkeldey, Stockmair & Schwanhäusser**  
**Anwaltssozietät**  
**Leopoldstrasse 4**  
**80802 München (DE)**

(54) **RADIOACTIVE RAY DETECTING METHOD AND DEVICE UTILIZING ENERGY AND POSITION INFORMATION**

(57) Upon detection of radiation by using a (three-dimensional) detector capable of distinguishing a detection position in a depth direction and energy, an energy window for distinguishing between a signal and noise is changed depending on the detection position in the depth direction, thus making it possible to obtain scattering components inside the detector. Alternatively, a weight is given to a detection event depending on the detection position in the depth direction and energy information to obtain scattering components inside the detector. Thereby, scattering components inside the detector can be obtained to increase the sensitivity of the detector. In this case, different detecting elements can be used depending on the detection position in the depth direction.

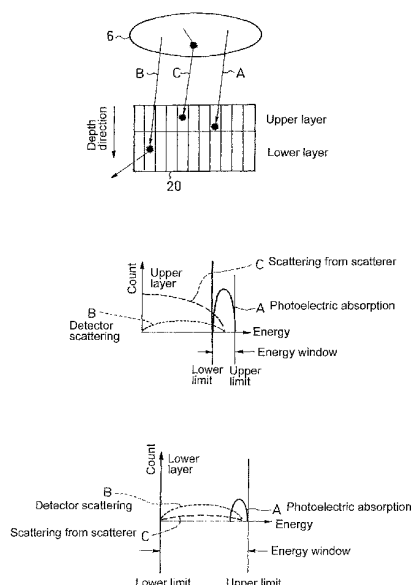Fig. 8



**EP 2 138 867 A1**

## Description

[Technical Field]

**[0001]** The present invention relates to a radiation detecting method and equipment thereof, and in particular to a radiation detecting method utilizing energy information and positional information preferably used in positron imaging equipment or positron emission tomography (PET) equipment and to the equipment thereof.

[Background Art]

**[0002]** As shown in Fig. 1, PET equipment is known in which positrons emitted from a positron emission nuclide 8 by the decay of  $+\beta$  undergo pair annihilation with surrounding electrons, and thus generated annihilation radiations 8a, 8b at 511 keV are determined by a pair of radiation detectors 10a, 10b according to the principle of coincidence. In this case, since only the annihilation radiations to which energy at 511 keV has been imparted are utilized, energy (signal) to be obtained is restricted for a lower limit and an upper limit by an energy window. Thereby, the position at which the nuclide 8 is present can be localized on one line segment connecting between the pair of detectors 10a, 10b (coincidence line: line-of-response: LOR). When an axis from the head of a body under testing to the feet is defined as a body axis, a distribution of the nuclide on a planar surface intersecting perpendicularly with the body axis is obtained by image reconfiguration in two-dimensional mode from data of the coincidence line determined on the planar surface in various directions.

**[0003]** A PET detector 10 is a collection of micro-detecting elements, the cross section of which is approximately 5 mm by 5 mm, and requires approximately 2 cm to 3 cm in thickness in order to detect at high probability a pair of annihilation radiations 8a, 8b oppositely emitted from the body. Further, in order to capture the pair of annihilation radiations, the detectors 10 are in general arranged in a ring shape so as to cover a subject, as shown in Fig. 2. However, radiation which is made incident obliquely into the detector 10 will cause a measurement error so as to deteriorate spatial resolution, for which there is no choice but to make the diameter of a ring much larger than the visual field.

**[0004]** In PET equipment, in order to acquire a higher detectability, a three-dimensional detector has been developed for detecting a depth position as well at which the radiation is made incident into a detecting element. As exemplified in Fig. 3, detecting elements of the same type 21 to 24 are stacked on a light receiving element 26, and an optical reflector placed between the detecting elements is used to control the path of light, thus making it possible to localize a depth detecting position and energy from a difference in signals output from the light receiving element 26 (refer to Japanese Published Unexamined Patent Application No. 2004-279057 (Patent

Document 1), H. Murayama, H. Ishibashi, H. Uchida, T. Omura, T. Yamashita, "Design of a depth of interaction detector with a PS-PMT for PET," IEEE Trans. Nucl. Sci., Vol. 47, No. 3, 1045-1050, 2000 (Non-patent Document 1)). Further, two layers are identified for depth in general by stacking two types of detecting elements for each layer to localize a depth detecting position from a time difference in signals output from the light receiving element 26.

**[0005]** The above-described three-dimensional detector 20 is able to improve the deterioration of spatial resolution resulting from radiation made incident obliquely into the detecting elements. Further, the detector 20 can be brought closer to a body under testing than a detector used in the conventional PET equipment, thereby performing detection at a higher sensitivity.

**[0006]** On the other hand, as a method for improving the sensitivity, there is presented an idea of utilizing detector scattering shown in Fig. 4(A). In a conventional two-dimensional detector 10, as shown in Fig. 4(B) and (C), the detector scattering cannot be distinguished from scattering from a body under testing (also referred to as a scatterer) 6. Therefore, as shown in Fig. 5 and Fig. 6, a lower limit of an energy window is adjusted to that of energy at photoelectric absorption A, by which both scattering events are eliminated as noises.

**[0007]** It is noted that, as shown in Fig. 7, a shield 12 for removing low-energy scattered radiation is installed on the upper face of the detector 10, thus making it possible to remove scattered radiation from the body under testing 6. However, the shield also removes partially a photoelectric absorption event (refer to G. Muehllheiner: "Position camera with extended counting rate capability," J. Nucl. Med. Vol. 16, 663-657, 1975 (Non-Patent Document 2)).

**[0008]** Thus, PET equipment on which three-dimensional detectors are mounted is able to adopt an arrangement of the detectors so as to give a higher sensitivity than the conventional PET equipment. Nevertheless, there is a disadvantage that a high sensitivity measurement method and a great amount of information that the PET equipment has in principle are not yet utilized to a full extent.

[Disclosure of the Invention]

**[0009]** The present invention has been made in order to solve the above disadvantage, an object of which is to obtain scattering components inside a detector which would be otherwise discarded, thereby improving the sensitivity of detection.

**[0010]** An event scattered in the body of a subject undergoes energy loss before being made incident into a detector, and as the event is decreased in energy more greatly than 511 keV at the time when the event is made incident into the detector, there is a higher probability that the event may impart all the energy on an upper layer of the detector and halt. On the other hand, an event scattered only at a detecting element has 511 keV in energy

at the time when the event is made incident, and scattered inside a crystal once or scattered repeatedly a plurality of times. Thereafter, the event will finally impart all the energy at 511 keV or will impart some of the energy and escape outside the detector, with the remaining energy retained. Where the event does not scatter in the body but imparts all the energy at 511 keV to a detecting element, the event is detected inside an energy window shown in Fig. 5. However, where the event imparts only some of the energy, the event may be out of the energy window despite the fact that it has useful positional information. Therefore, in the conventional PET equipment, as shown in Fig. 4, a true coincidence B scattered inside a detector or a scatter coincidence C cannot be identified, whereby the coincidence B having useful positional information for the most part has been discarded.

**[0011]** As shown in Fig. 8, since the three-dimensional detector 20 is able to reduce scattering from a scatterer (scatter coincidence) C at detecting elements on a lower layer, the detector 20 is able to utilize as a coincidence the detector scattering B as well by decreasing a lower limit of the energy window to a lower limit of detector scattering energy. The present invention is to provide a method in which the above-described events are effectively utilized to improve the sensitivity of radiation detecting equipment. A ratio of detector scattering to scattering from a body under testing is expected to be different depending on the depth at which radiation is detected and energy imparted. Therefore, if a detection position in a depth direction detected by a three-dimensional detector and energy information can be obtained, it is possible to obtain scattering components inside the detector at a region excluding that large in scattering components from a body under testing. Further, when a detection position in a depth direction detected by the three-dimensional detector and energy information are obtained, energy large in scattering components from the body under testing is decreased in weight and energy few in scattering components from the body under testing is increased in weight to acquire data, thus making it possible to obtain scattering components inside the detector, while a mixture ratio of scattering components from the body under testing is minimized.

**[0012]** The present invention has been made, with attention given to the above description, and has solved the problem by procedures in which upon detection of radiation by using a detector capable of distinguishing a detection position in a depth direction and energy, an energy window for distinguishing between a signal and noise is changed depending on the detection position in the depth direction, thus making it possible to obtain scattering components inside the detector.

**[0013]** Further, the present invention is to provide radiation detecting equipment which detects radiation by using a detector capable of distinguishing a detection position in a depth direction and energy, and the radiation detecting equipment utilizing energy information and positional information in which an energy window for distin-

guishing between a signal and noise is changed depending on a detection position in a depth direction, thus making it possible to obtain scattering components inside the detector.

**[0014]** In this case, the present invention is able to provide different detecting elements depending on a detection position in a depth direction.

**[0015]** The present invention has solved the above problem by procedures in which upon detection of radiation by using a three-dimensional detector capable of distinguishing a detection position in a depth direction and energy, a weight is given to a detection event depending on the detection position in the depth direction and energy information, thus making it possible to obtain scattering components inside a detector.

**[0016]** According to the present invention, scattering components inside a detector can be obtained to increase the sensitivity of the detector. Thereby, PET equipment, positron imaging equipment and others can be increased in sensitivity.

**[0017]** Further, a weight is given to a detection event depending on a detection position in a depth direction and energy information to utilize more detailed energy information, by which a mixture ratio of scattering from an object (scatterer) is reduced to utilize a detector scattering event and improve a signal to noise ratio.

[Brief Description of the Drawings]

**[0018]**

Fig. 1 is a view showing a principle of PET equipment.

Fig. 2 is a view showing a whole constitution of the conventional PET equipment.

Fig. 3 is a perspective view showing a three-dimensional detector presented in Patent Document 1.

Fig. 4 is a view showing interactions of gamma rays and energy spectrum for describing a principle of the present invention.

Fig. 5 is a view showing a method for removing scattered radiation by a conventional energy window.

Fig. 6 is a view showing data processing by a conventional method.

Fig. 7 is a view showing a method for removing scattered radiation by a conventional shield.

Fig. 8 is a view showing the principle of the present invention.

Fig. 9 is a view showing a first embodiment of PET equipment in which the present invention is utilized.

Fig. 10 is a flow chart showing data processing procedures of the first embodiment.

Fig. 11 is a view showing a state of radiation made incident of the first embodiment.

Fig. 12 is a flow chart showing coincidence procedures of the first embodiment.

Fig. 13 is a view showing a second embodiment of the PET equipment utilizing the present invention.

Fig. 14 is also a flow chart showing processing procedures of a third embodiment.

Fig. 15 is also a flow chart showing processing procedures in a fourth embodiment.

Fig. 16 is a view showing an energy window of the embodiments.

Fig. 17 is a view showing an energy spectrum of (A) true coincidence and that of (B) scattered coincidence in a comparative manner.

Fig. 18 is also a view showing (A) sensitivity and (B) scatter fraction in a comparative manner.

#### [Best Mode for Carrying Out the Invention]

**[0019]** Hereinafter, a description will be given in detail for embodiments of the present invention by referring to the drawings.

**[0020]** A first embodiment of the present invention is PET equipment or the like on which, as shown in Fig. 9, a three-dimensional detector 20 is mounted, and the PET equipment in which, as shown in Fig. 10, a detection depth is limited at a lower energy region as well to utilize detector scattering and, as shown in Fig. 11, a mechanism is provided for distinguishing between an event C scattered inside a body under testing 6 and an event B which imparts a portion of energy to the detector 20 after scattering inside the detector 20. Thereby, the PET equipment or the like having a three-dimensional detector can be further increased in sensitivity, while the deterioration of positional information is prevented.

**[0021]** Fig. 12 shows procedures of coincidence.

**[0022]** Further, in the present invention, the need is eliminated for using detecting elements of the same type on all layers when the detecting elements are stacked. As described in the second embodiment shown in Fig. 13, an inexpensive detecting element 20B lower in effective atomic number is used on a lower layer unlike on an upper layer which requires an expensive detecting element 20A higher in effective atomic number, thus making it possible to use different types of detecting elements. In this case, the detecting element 20A on the upper layer is made long enough in length to stop scattered radiation but made shorter in length than the detecting element 20B on the lower layer, thereby realizing PET equipment lower in cost but higher in performance.

**[0023]** Alternatively, it is possible to increase the sensitivity of PET equipment in which only detecting elements lower in effective atomic number such as semiconductor detectors are used.

**[0024]** A third embodiment of the present invention is PET equipment or the like on which, as shown in Fig. 9, a three-dimensional detector 20 is mounted, and in which as shown in Fig. 14, a weight is given to a detection event depending on a detection position and energy, thereby acquiring histograms.

**[0025]** Further, as shown in Fig. 15, a fourth embodiment is that in which a detection event is stored as list mode data and, on image reconfiguration, a weight is

given to a detection position and energy, thereby performing the reconfiguration.

**[0026]** In this case, as shown in Fig. 8, a ratio of detector scattering to scattering from a scatterer at a low energy region is calculated in advance by simulation or the like, thereby tabulating a weighting depending on a detection depth (layer) and energy. The weight is set in proportion to a ratio of detector scattering to scattering from a scatterer, for example. Alternatively, in a case where a ratio of detector scattering to scattering from a scatterer is in excess of a predetermined value, calculation is made by setting the ratio to 1.0. In other cases, the calculation is made by setting the ratio to 0.0.

**[0027]** As described in the third and fourth embodiments, more detailed energy information is utilized than in the first or second embodiment, by which a mixture ratio of scattering from an object (scatterer) is reduced to effectively use a detector scattering event and also to improve a signal to noise ratio.

**[0028]** A simulation was performed by using the test model of PET equipment for the head developed by the applicant and others "jPET-D4" (referto E. Yoshida, K. Kitamura, T. Tsuda, et. al. : "Energy spectra analysis of four-layer DOI detector for brain PET scanner: jPET-D4," Nucl. Instr. Meth. A, 577, 664-669, 2006 (Non-Patent Document 3)). In this equipment, three-dimensional detectors 20 each of which is made up of four stacked layers of a GSO scintillator measuring 2.9 mm x 2.9 mm x 7.5 mm were used to constitute a detector ring measuring 39 cm in ring diameter and 26 cm in length. As a phantom simulating a body under testing 6, a cylindrical phantom measuring 20 cm in diameter and 20 cm in length was filled with water and a pair of 20 cm-across linear radiation sources which emit a pair of radiation at 511 keV were installed on the central axis.

**[0029]** In a conventional method, energy windows are the same on all layers, for example, 400 to 600 keV. However, in a method according to the present invention, as shown in Fig. 16, an energy window from 400 to 600 keV was provided on a first layer, while two energy windows from 100 to 300 keV and 400 to 600 keV were provided on a second to a fourth layer. More specifically, provided was an energy window from 100 to 600 keV excluding a range from 300 to 400 keV. As described above, a plurality of energy windows may be installed whenever necessary, which is different from the conventional PET equipment.

**[0030]** Fig. 17 shows an energy spectrum of (A) true coincidence and that of (B) scatter coincidence. It is apparent that as the layer goes further down, influence of scattered radiation from a body under testing shown in (B) is reduced.

**[0031]** Fig. 18 shows a change in (A) relative sensitivity and (B) scatter fraction (ratio at which object scattering is contained in measured data) when the lower limit of an energy window is changed. In the relative sensitivity, the lower limit 400 keV of the energy window is given as 100. As apparent from this drawing, the present invention

is able to provide a higher sensitivity while suppressing an increase in scatter fraction.

**[0032]** In the previous description, the present invention is applied to PET equipment. However, the present invention shall not be limited thereto but may be applied to other nuclear medical imaging equipment such as positron imaging equipment and also to radiation detecting equipment in general. Further, the three-dimensional detector shall not be limited to the type shown in Fig. 3 and also acceptable is that which is able to distinguish a position in a depth direction in an analog manner.

[Industrial Applicability]

**[0033]** The present invention is applicable to nuclear medical imaging equipment such as positron imaging equipment and also to radiation detecting equipment in general, in addition to PET equipment.

### Claims

1. A radiation detecting method utilizing energy information and positional information, wherein upon detection of radiation by using a detector capable of distinguishing a detection position in a depth direction and energy, an energy window for distinguishing between a signal or noise is changed depending on the detection position in the depth direction, thus making it possible to obtain scattering components inside the detector.
2. The radiation detecting method utilizing energy information and positional information according to claim 1, wherein different detecting elements are used depending on a detection position in a depth direction.
3. Radiation detecting equipment which detects radiation by using a detector capable of distinguishing a detection position in a depth direction and energy, the radiation detecting equipment utilizing energy information and positional information, wherein an energy window for distinguishing between a signal and noise is changed depending on a detection position in a depth direction, thus making it possible to obtain scattering components inside the detector.
4. The radiation detecting equipment utilizing energy information and positional information according to claim 3, wherein different detecting elements are provided depending on a detection position in a depth direction.
5. The radiation detecting equipment according to claim 3 or claim 4, wherein information on radiation of two or more energy windows few in scattering components is utilized for monoenergetic radiation, depending on a detection position in a depth direction.
6. Radiation detecting method utilizing energy information and positional information, wherein upon detection of radiation by using a detector capable of distinguishing a detection position in a depth direction and energy, a weight is given to a detection event depending on the detection position in the depth direction and energy information, thus making it possible to obtain scattering components inside the detector.
7. The radiation detecting method utilizing energy information and positional information according to claim 6, wherein different detecting elements are used depending on a detection position in a depth direction.
8. Radiation detecting equipment which detects radiation by using a detector capable of distinguishing a detection position in a depth direction and energy, the radiation detecting equipment utilizing energy information and positional information, wherein a weight is given to a detection event depending on the detection position in the depth direction and the energy information, thus making it possible to obtain scattering components inside the detector.
9. The radiation detecting equipment utilizing energy information and positional information according to claim 8, wherein different detecting elements are provided depending on a detection position in a depth direction.

Fig. 1

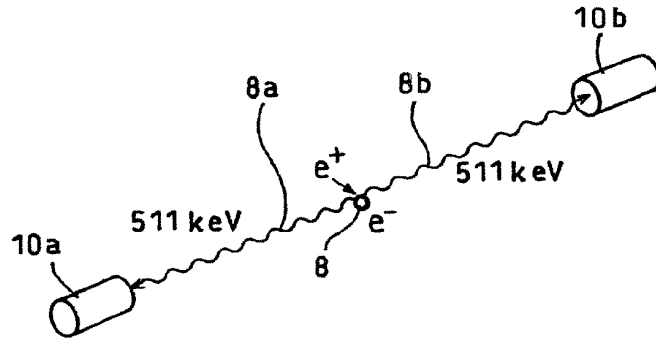


Fig. 2

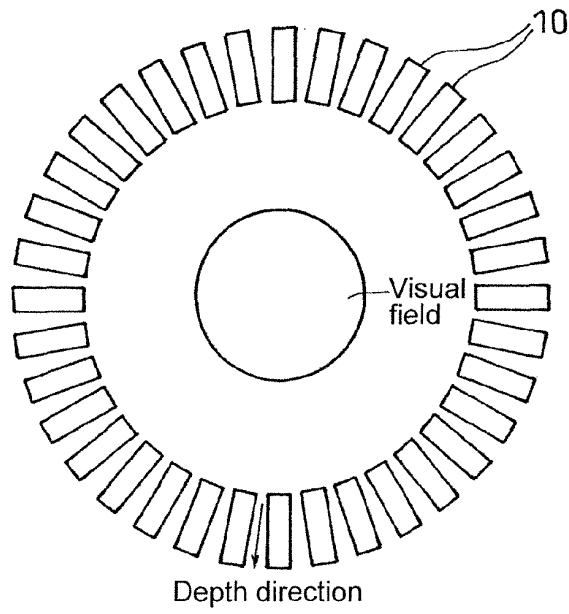


Fig. 3



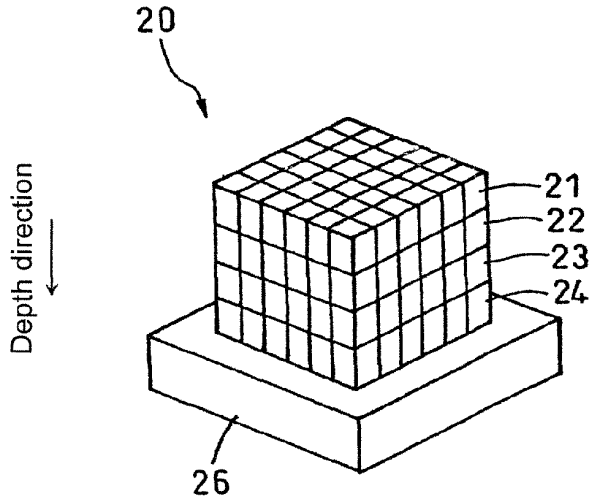


Fig. 4

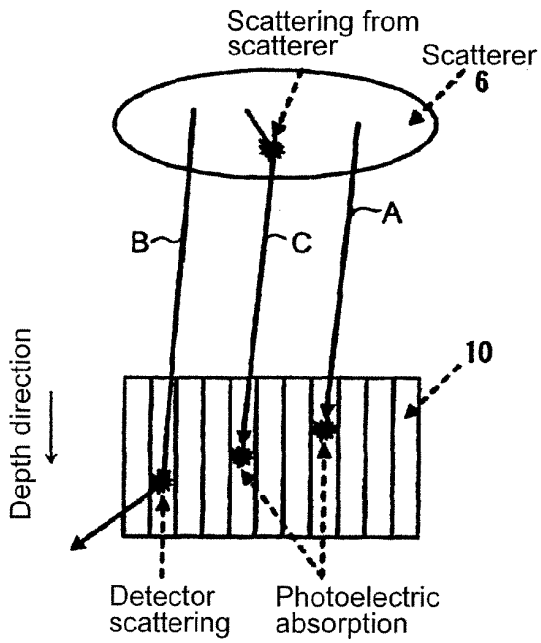(A) Interactions with gamma rays



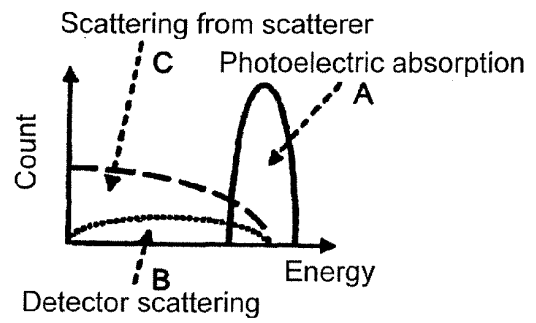(B) Energy spectrum by each interaction



(C) Whole energy spectrum



Fig. 5

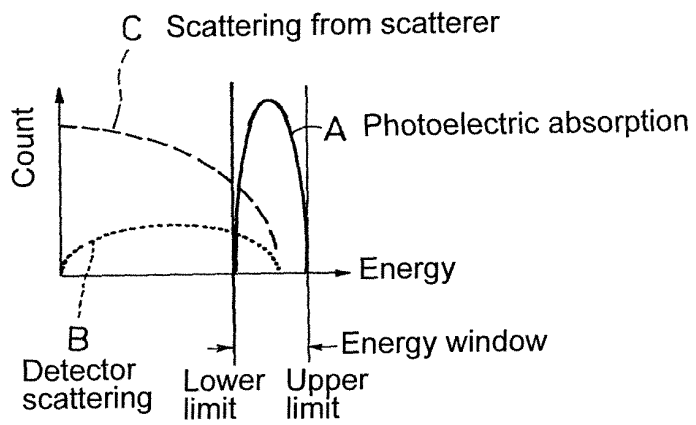
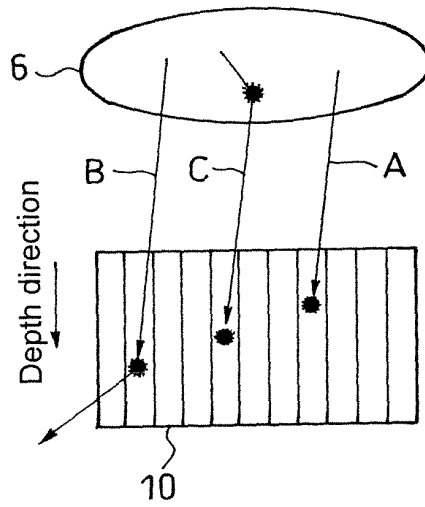




Fig. 6

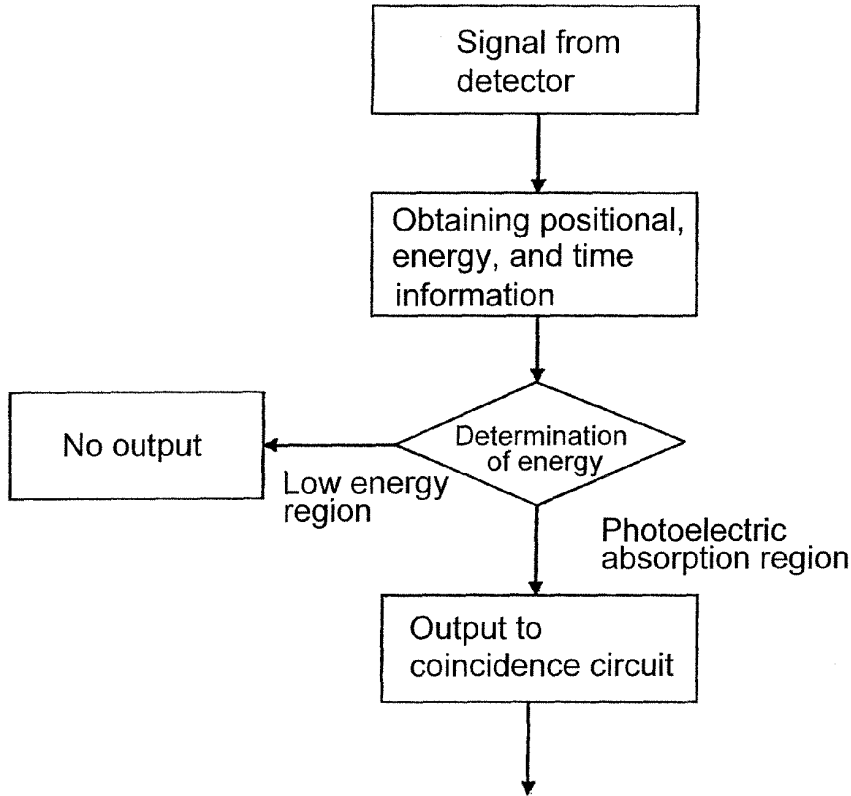


Fig. 7

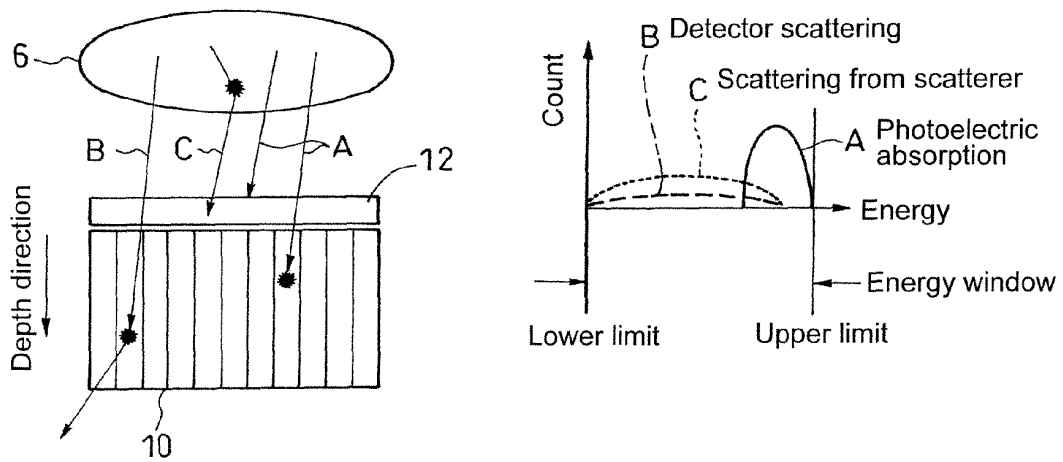


Fig. 8

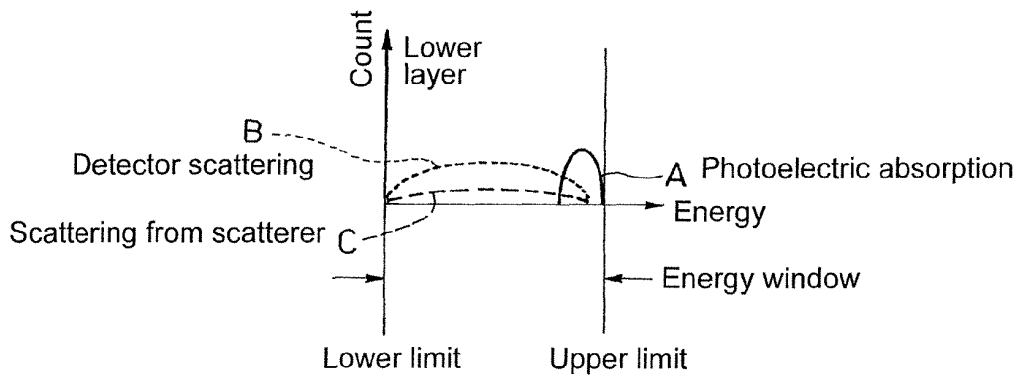
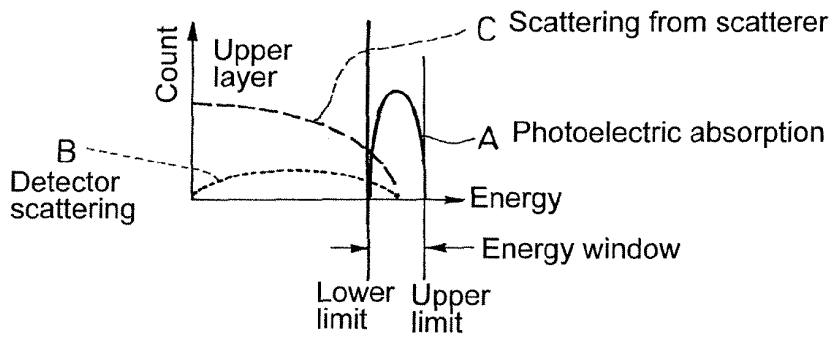
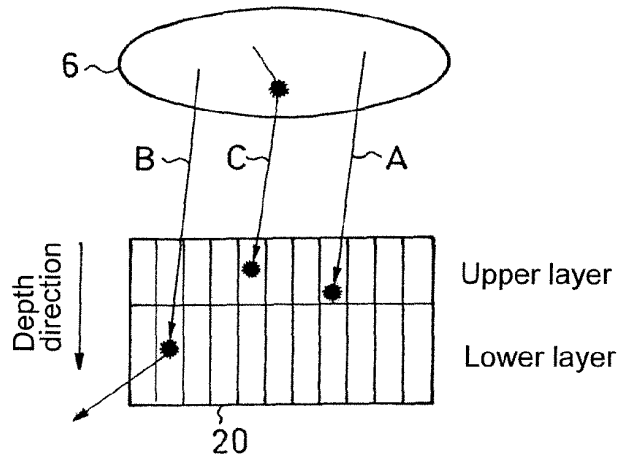


Fig. 9

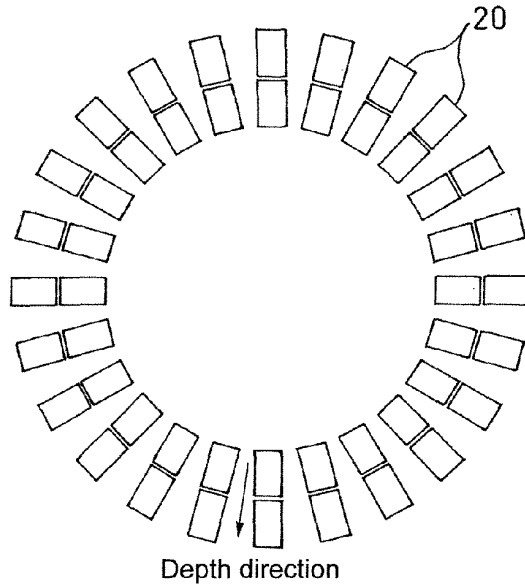


Fig. 10

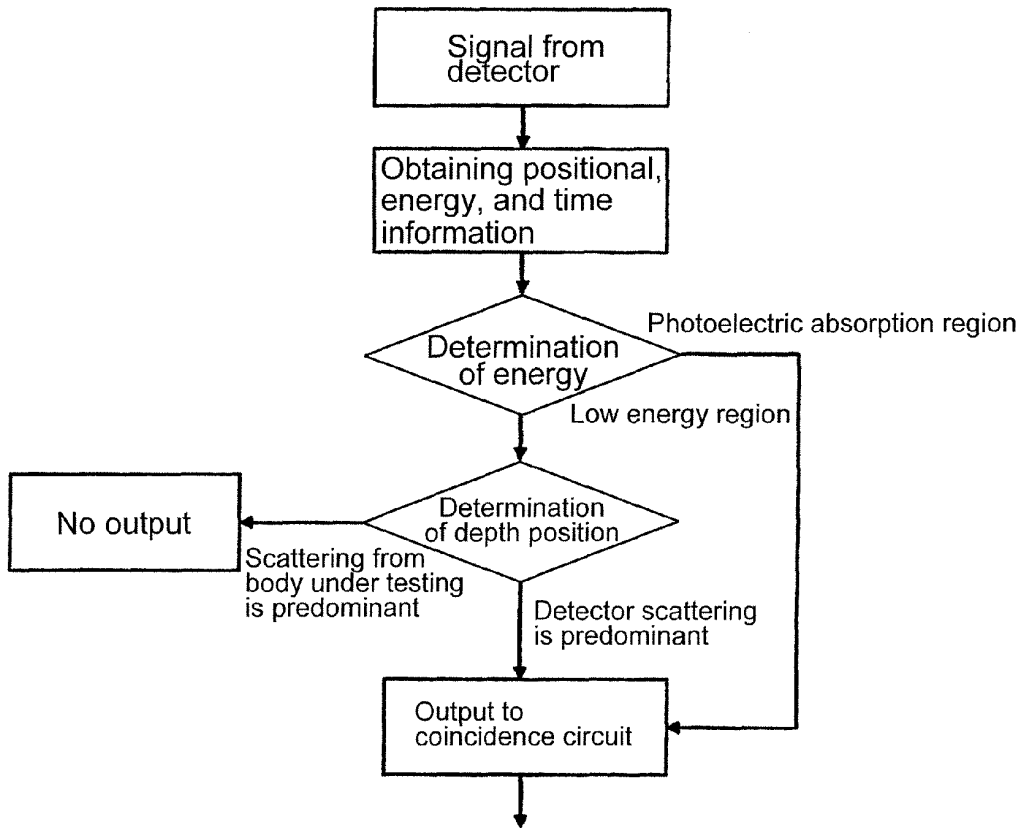


Fig. 11

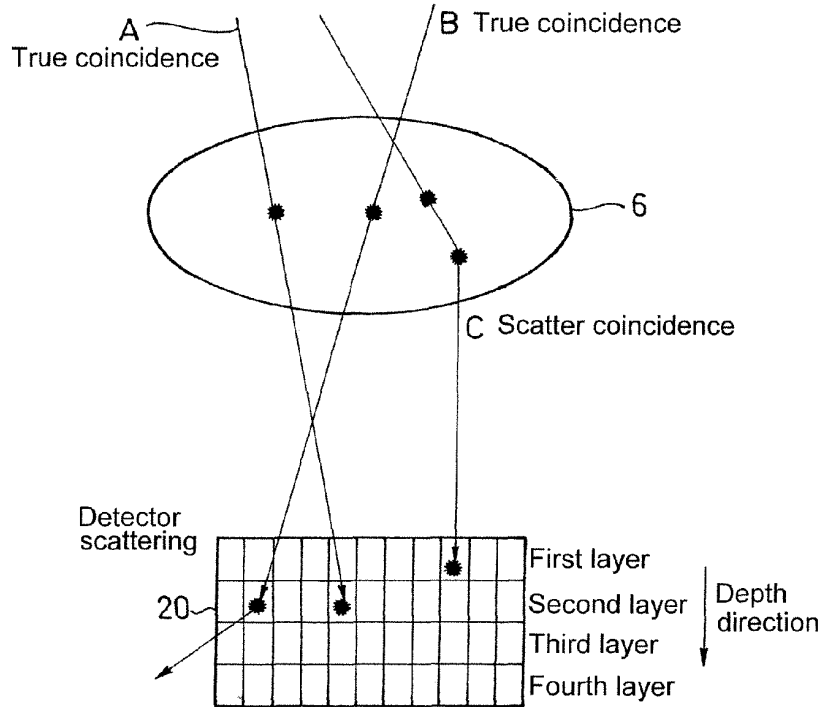


Fig. 12

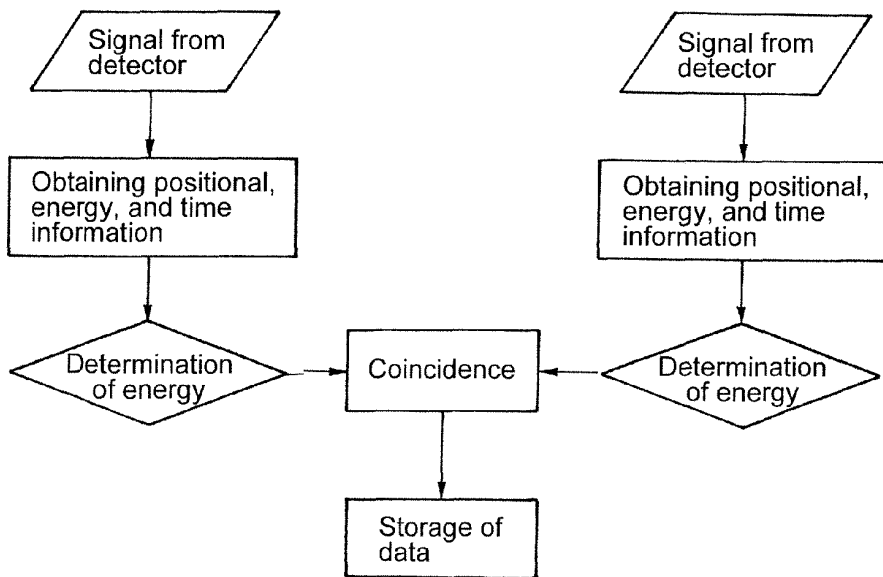


Fig. 13

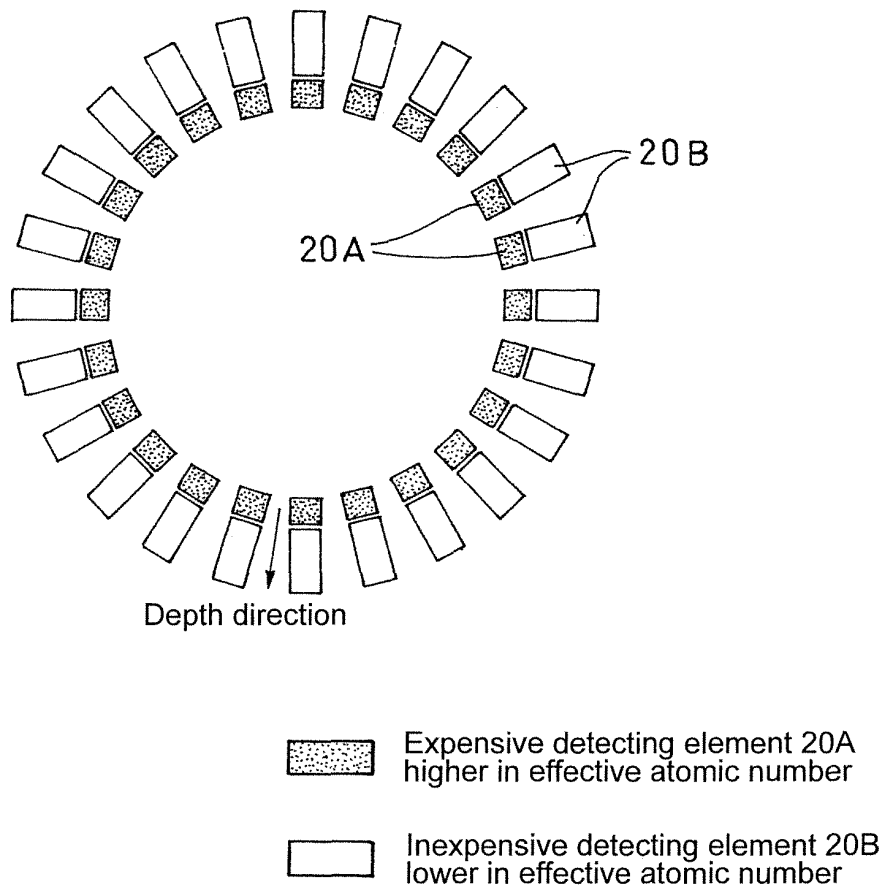


Fig. 14

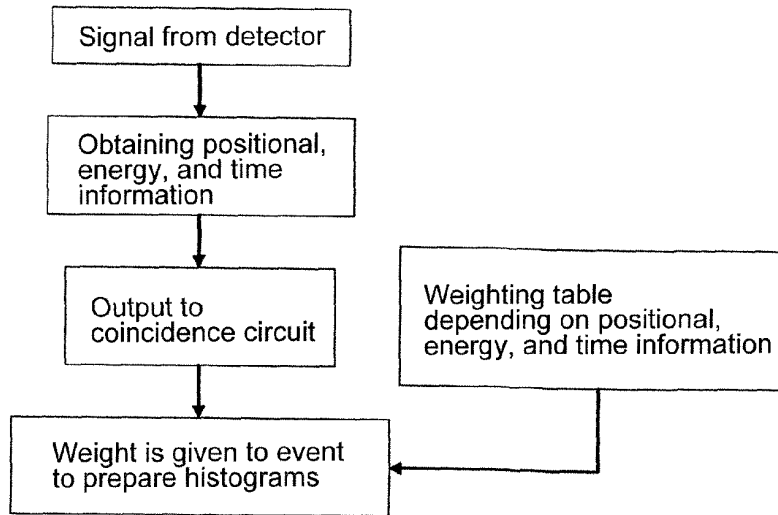


Fig. 15

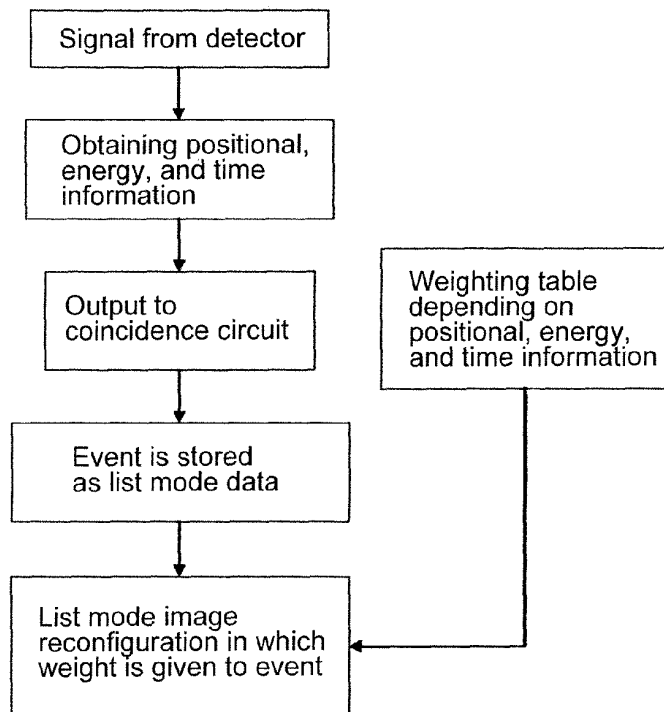


Fig. 16


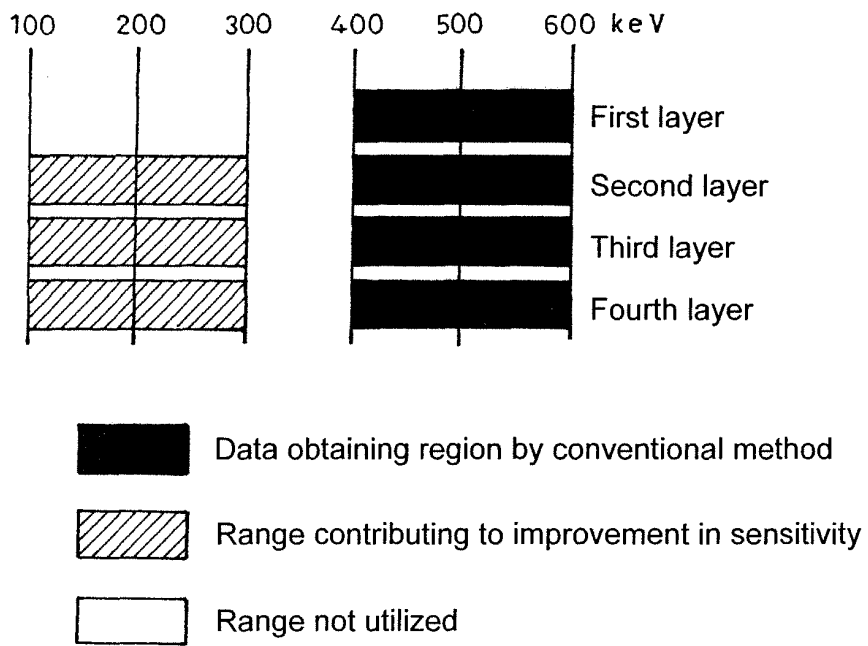


Fig. 17

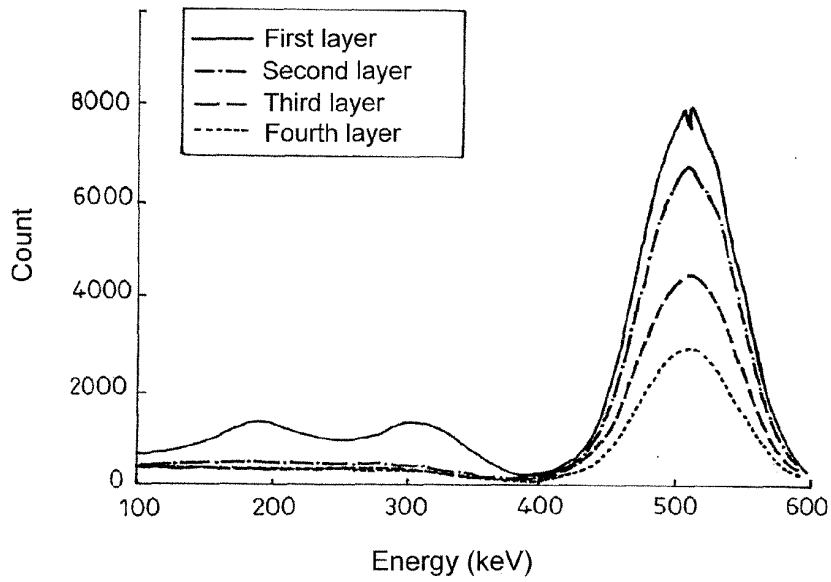(A) Energy spectrum of true coincidence



(B) Energy spectrum of scatter coincidence

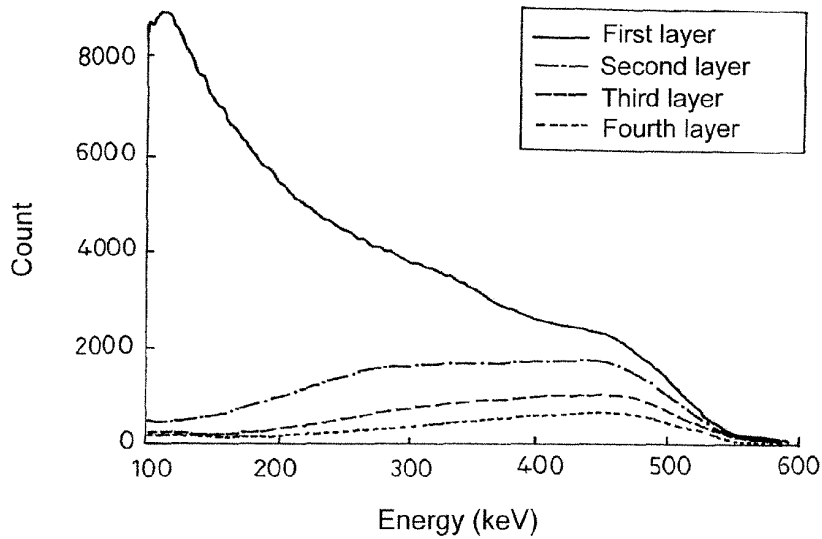
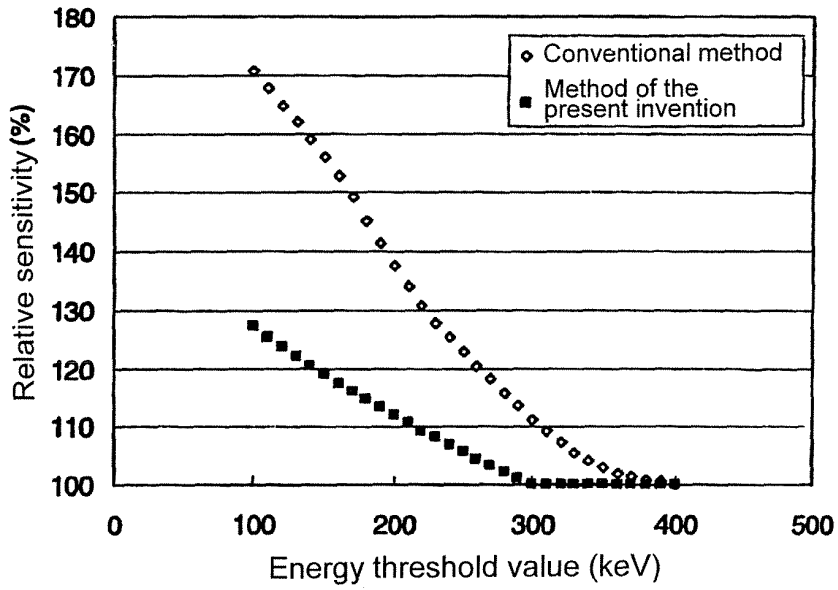


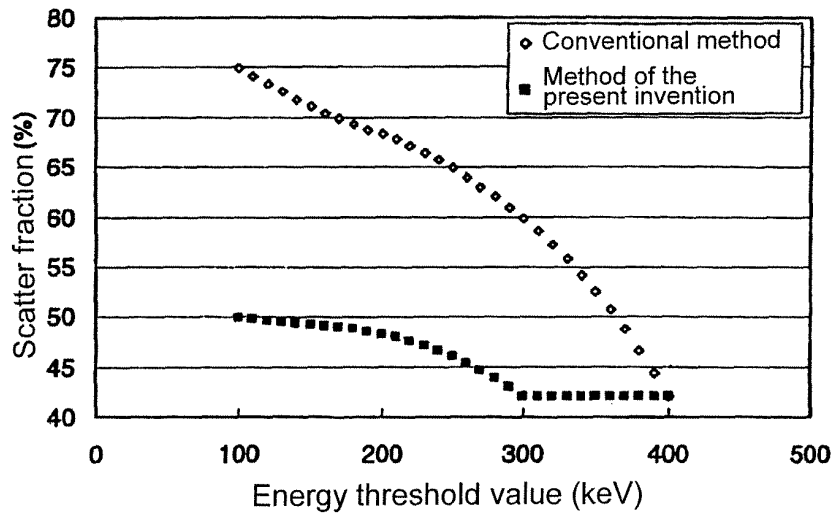


Fig. 18

(A) Sensitivity



(B) Scatter fraction



## INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP2007/066940

A. CLASSIFICATION OF SUBJECT MATTER G01T1/20(2006.01)i, G01T1/161(2006.01)i		
According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED		
Minimum documentation searched (classification system followed by classification symbols) G01T1/00-7/12		
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Jitsuyo Shinan Koho 1922-1996 Jitsuyo Shinan Toroku Koho 1996-2007 Kokai Jitsuyo Shinan Koho 1971-2007 Toroku Jitsuyo Shinan Koho 1994-2007		
Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) JSTPlus (JDream2)		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X A	JP 62-203078 A (Shimadzu Corp.), 07 September, 1987 (07.09.87), Page 1, right column, line 5 to page 2, lower left column, line 9 (Family: none)	1-4, 6-9 5
<input type="checkbox"/> Further documents are listed in the continuation of Box C. <input type="checkbox"/> See patent family annex.		
* Special categories of cited documents: "A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family		
Date of the actual completion of the international search 13 September, 2007 (13.09.07)		Date of mailing of the international search report 25 September, 2007 (25.09.07)
Name and mailing address of the ISA/ Japanese Patent Office		Authorized officer
Facsimile No.		Telephone No.

Form PCT/ISA/210 (second sheet) (April 2005)

INTERNATIONAL SEARCH REPORT

International application No.  
PCT/JP2007/066940

<b>Box No. II</b>		<b>Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)</b>
<p>This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:</p> <p>1. <input type="checkbox"/> Claims Nos.: because they relate to subject matter not required to be searched by this Authority, namely:</p> <p>2. <input type="checkbox"/> Claims Nos.: because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:</p> <p>3. <input type="checkbox"/> Claims Nos.: because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).</p>		
<b>Box No. III</b>		<b>Observations where unity of invention is lacking (Continuation of item 3 of first sheet)</b>
<p>This International Searching Authority found multiple inventions in this international application, as follows:</p> <p>The common matter of the invention according to claims 1 - 5, i.e., "a radioactive ray detecting method (device) enabled to acquire a scattered component in a detector, by changing an energy window" is not the special technical feature, since it is not novel because it was disclosed in document: JP 62-203078 A (Shimadzu Corp.), 7 September, 1987 (07.09.87), line 5, right column, page 1 to line 9, lower left column, page 2.</p> <p>The common matter of the invention according to claims 6 - 9, i.e., "a radioactive ray detecting method (device) enabled to acquire a scattered component in a detector, by weighting a detection event according to a detection position in a depth direction (Continued to extra sheet.)</p> <p>1. <input type="checkbox"/> As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.</p> <p>2. <input checked="" type="checkbox"/> As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.</p> <p>3. <input type="checkbox"/> As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:</p> <p>4. <input type="checkbox"/> No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:</p> <p><b>Remark on Protest</b></p> <p><input type="checkbox"/> The additional search fees were accompanied by the applicant's protest and, where applicable, payment of a protest fee.</p> <p><input type="checkbox"/> The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.</p> <p><input type="checkbox"/> No protest accompanied the payment of additional search fees.</p>		

Form PCT/ISA/210 (continuation of first sheet (2)) (April 2005)

INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP2007/066940

Continuation of Box No.III of continuation of first sheet(2)

and an energy information" is not the special technical feature, too, since it is not novel because it was disclosed in the aforementioned document .